

# Unilateral Outer Bow Expanded Cervical Headgear Force System: 3D Analysis Using Finite Element Method

Allahyar Geramy<sup>1✉</sup>, Omid Mortezaei<sup>2</sup>, Masomeh Esmaily<sup>3</sup>, Hojat Darvishpour<sup>4</sup>

<sup>1</sup>Professor, Dental Research Center Dentistry Research Institute, Department of Orthodontics, Tehran University of Medical Sciences, Tehran, Iran

<sup>2</sup>Assistant Professor of orthodontics, Dental Caries Prevention Research Center, Qazvin University of Medical Sciences, Qazvin, Iran

<sup>3</sup>Assistant Professor, Department of Orthodontics, Lorestan University of Medical Sciences, Khorramabad, Iran

<sup>4</sup>Post graduate student, Orthodontics Department, School of Dentistry, Tehran University of Medical Sciences, Tehran, Iran

## Abstract

**Objectives:** Headgears are among the effective orthodontic appliances to achieve treatment goals. Unilateral molar distal movement is sometimes needed during an orthodontic treatment, which can be achieved by an asymmetric headgear. Different unilateral headgears have been introduced. The main goal of this study was to analyze the force system of unilateral expanded outer bow asymmetric headgears by the finite element method (FEM).

**Materials and Methods:** Six 3D finite element models of a mesiodistal slice of the maxilla containing upper first molars, their periodontal ligaments (PDLs), cancellous bone, cortical bone, and a cervical headgear with expanded outer bow attached to maxillary first molars were designed in SolidWorks 2010 and meshed in ANSYS Workbench ver. 12.1. The models were the same except for the degree of outer bow expansion. The outer bow ends were loaded with 2-Newton force. The distal driving force and the net moment were evaluated.

**Results:** A decrease in the distalizing force in the normal side molar from 1.69 N to 1.37 N was shown by increasing the degree of unilateral expansion. At the same time, the force increased from 2.19 N to 2.49 N in the expanded side molar. A net moment increasing from 2.26 N.mm to 4.64 N.mm was also shown.

**Conclusion:** Unilateral outer bow expansion can produce different distalizing forces in molars, which increase by increasing the expansion.

**Keywords:** Extraoral Traction Appliances; Asymmetric; Finite Element Analysis

*Journal of Dentistry, Tehran University of Medical Sciences, Tehran, Iran (2015; Vol. 12, No. 4)*

✉ Corresponding author:  
A. Geramy, Department of  
Orthodontics, Tehran University  
of Medical Sciences, Tehran,  
Iran


gueramy@tums.ac.ir

Received: 27 June 2014  
Accepted: 26 January 2015


## INTRODUCTION

Headgear is a well-known and useful appliance in orthodontic treatments. Several techniques use headgear as an auxiliary appliance for orthodontic treatment with different objectives [1-4]. Norman Kingsley is known as the earliest documented user of headgear [5].

It was revived by Oppenheim who described its mechanical principles after being ignored by Angle. Armstrong in 1971 published a comprehensive study in headgear [6] which was followed by other researchers [7-11]. The significant effects of inner bow length on treatment results were assessed in a recent study by Geramy et al. who explained the dif-

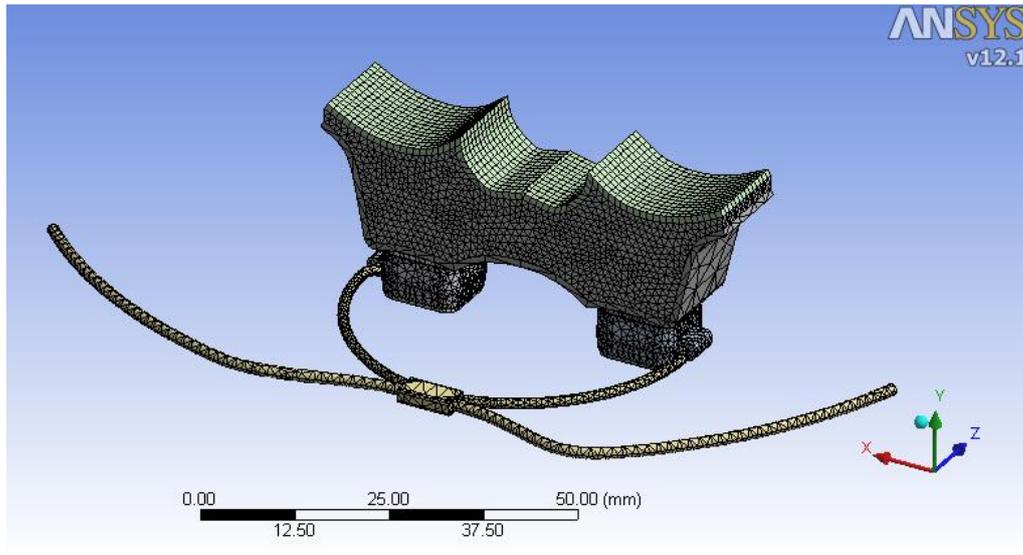

**Fig1a.** The meshed 3D model.

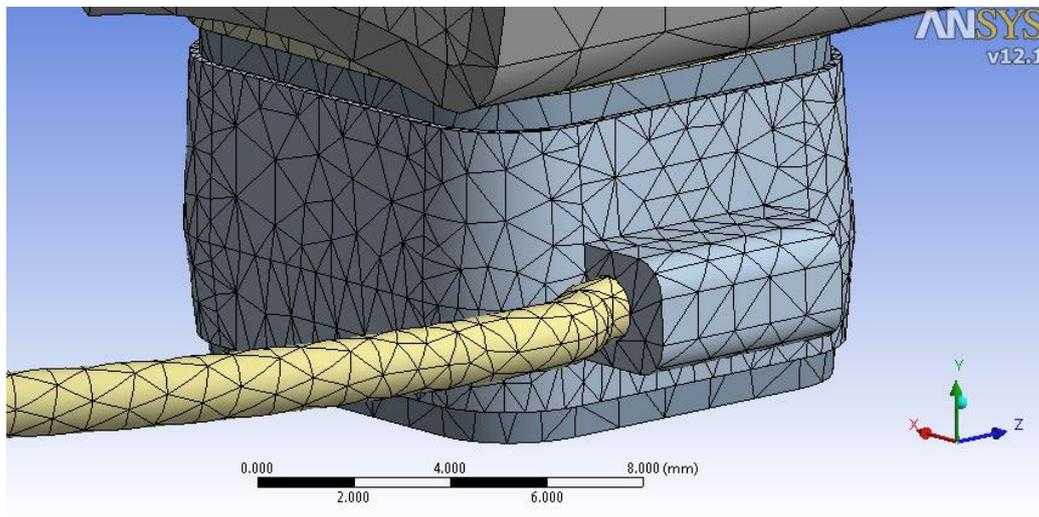

**Fig 1b.** Closer view of the 3D model showing the connection between the upper left molar, its band, and inner bow end.

ference in the resultant force when adjusting a symmetric cervical headgear in a mediolateral asymmetric molar position [12]. They reported different distal driving forces in different mediolateral molar positions. Different amounts of distal tooth movements are frequently required during treatment. Asymmetric force production has been the goal of different researchers [13-17].

Finite element method (FEM), as a numerical means of finding accurate answers to different questions, was introduced less than a century

ago in aerospace industry and soon found its way through the biological sciences.

This method has proven its efficiency in different lines of investigations and questions [18-23].

The main goal of this study was to assess the effects of a unilateral outer bow expanded headgear on producing an asymmetric force to the molars. In other words, this study tried to evaluate the nature of movements of upper first molars when loaded by a cervical headgear with a unilaterally expanded outer bow.

## MATERIALS AND METHODS

Six 3D finite element models of a mesiodistal slice of the maxilla containing upper first molars, their PDL, cancellous bone, cortical bone, stainless steel molar bands fitted to molar crowns, and a cervical headgear were designed. The models were the same except for the outer bow form, which was symmetric in model one and unilaterally (right side) expanded in models 2 through 5. The right outer bow expansion was designed considering an arc drawn with the center in the anterior most point of the outer bow.

Four different positions of the symmetric outer bow and the most expanded one were designed by dividing the angle difference between two extreme (the symmetric position and the most expanded one) outer bow positions. In this way, the gradual expansions of the outer bow were almost the same between models 2 to 5. Wire diameter was 1.6 mm in the outer bow and 0.9 mm in the inner bow (Figure 1). Due to the complexity of the molar shape, the results cannot be shown easily in the molar teeth. To solve this problem, molars were replaced by cubic parts in the last model to make it easy to show the displacements.(model 6)

The models were designed in SolidWorks 2006 (SolidWorks Corp., MA, USA) and were then transferred to ANSYS Workbench ver. 12.1 (ANSYS, Inc., PA, USA) for the solving process. To find the angles formed between the outer bow and its tangent to the neck, accurate trigonometric calculations were made using SolidWorks.

Linear measurements were required to draw Figure 2 and were derived from a volunteer dental student using a clinical vernier.

In this way, the exact force components in the anteroposterior and mediolateral directions were found which were later used in the ANSYS Workbench for the analysis phase. Static analysis was done using force components found in the previous stage. The outer bow bending under loading was analyzed.

In the final phase (model 6), the teeth were replaced in the model 5 with two blocks to simplify presenting the displacement patterns. Headgear was considered to be made of stainless steel. Meshing was done by a meshing program in Workbench. Meshed models contained 142,486 nodes and 84,023 elements (Figure 1). Outer bow ends were loaded with a 2 N force in the horizontal plane decomposed in mediolateral and anteroposterior directions. The mechanical properties of the materials used in the models were defined. (Table 1) The distalizing force to molars and moments were evaluated.

The other part of this study involved finding the best position of the center of outer bow bending. In other words, a geometrical method was considered to find the center point of the favorable arc to place the outer bow in its most asymmetric position when expanded (Figure 2a).


## RESULT

### *Distal component of force:*

Force components to distalize molars were the same in the symmetric outer bow (= 1.9588 N in the left side and 1.9588 N in the right side). Proceeding towards outer bow expansion models, a difference between right and left side molar force findings was found. The outer bow expansion side (= right side) force increased gradually in models from the 2nd model through the 5th one. The force was -2.1974N in the 2nd model and increased to -2.4916 N in the 5th model (the negative sign shows the distal direction of force). At the same time, the force pattern in the normal side molar showed a descending trend from model 2 to 5 from -1.6984 N to -1.3789 N. The force findings patterns are shown in Table 2 (Figure 3).

### *Moments:*

Positive sign moments are clockwise while the negative ones are counterclockwise (based on the view of Figure 2).

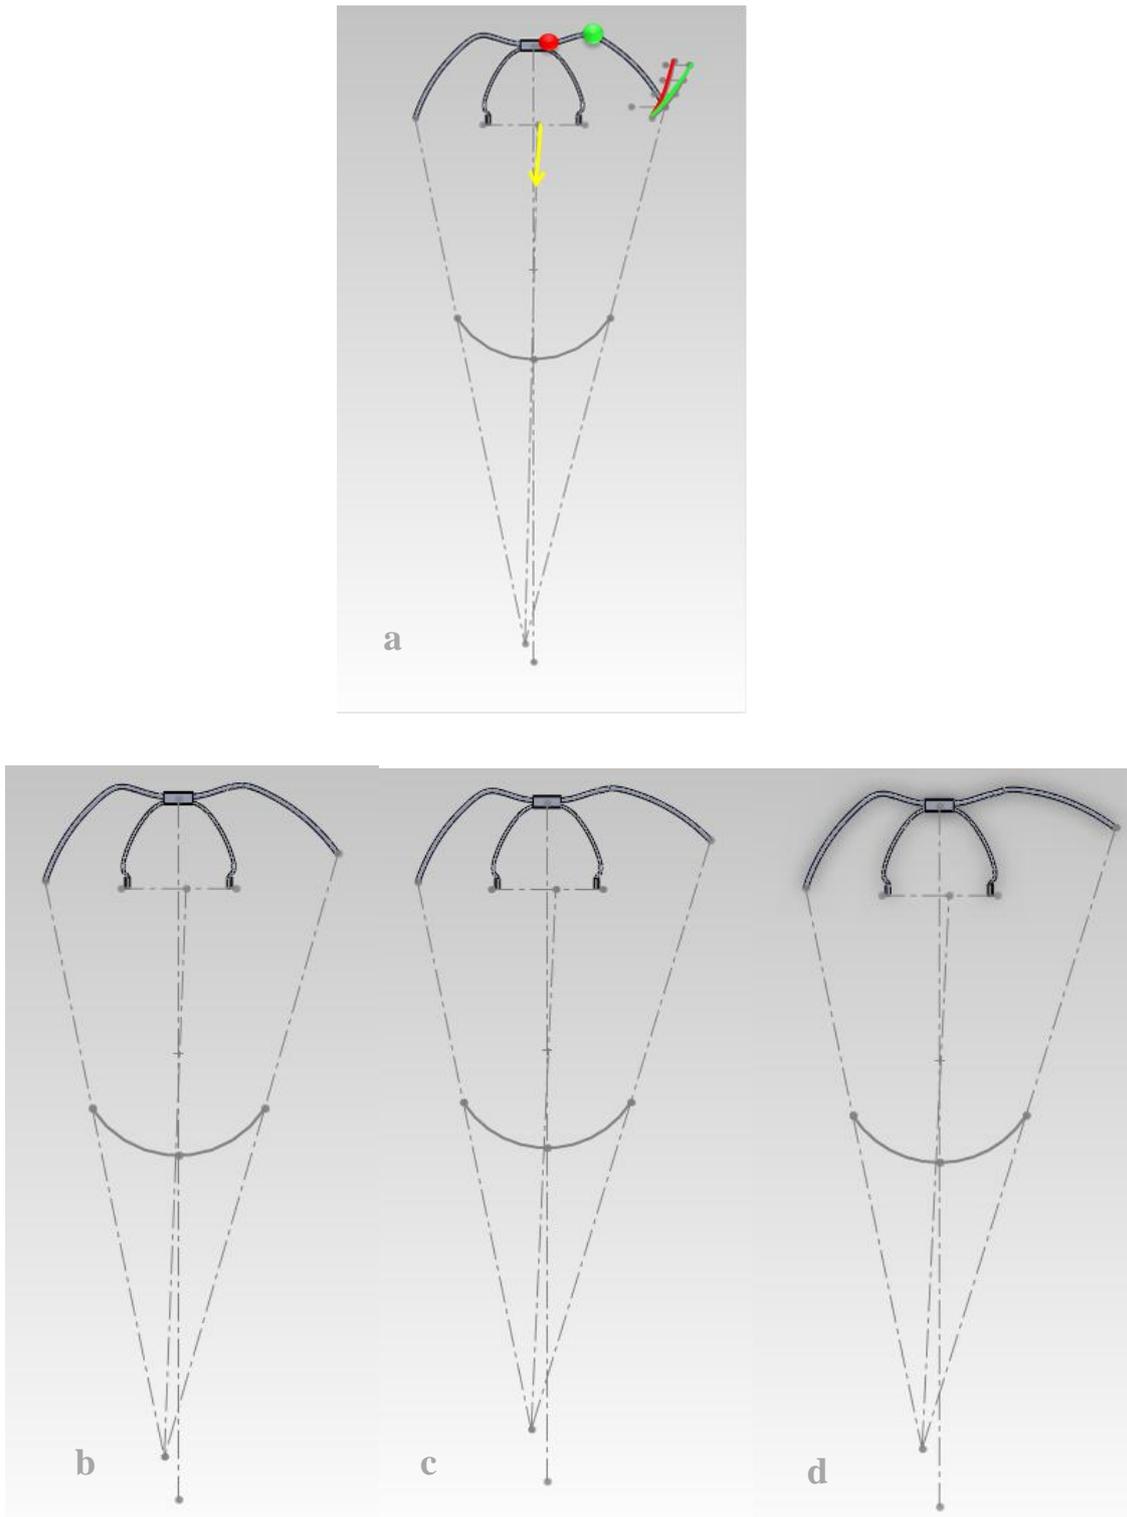

**Fig 2.** Four asymmetric headgear models produced by expansion of the outer bow. a) The green curve is selected for the outer bow expansion (with the green point as the center) which can produce a greater difference in the neck tangent line angles than the red curve with the red point as the center. The yellow vector shows the asymmetric force production. b, c, and d) Progressive steps of outer bow expansion.

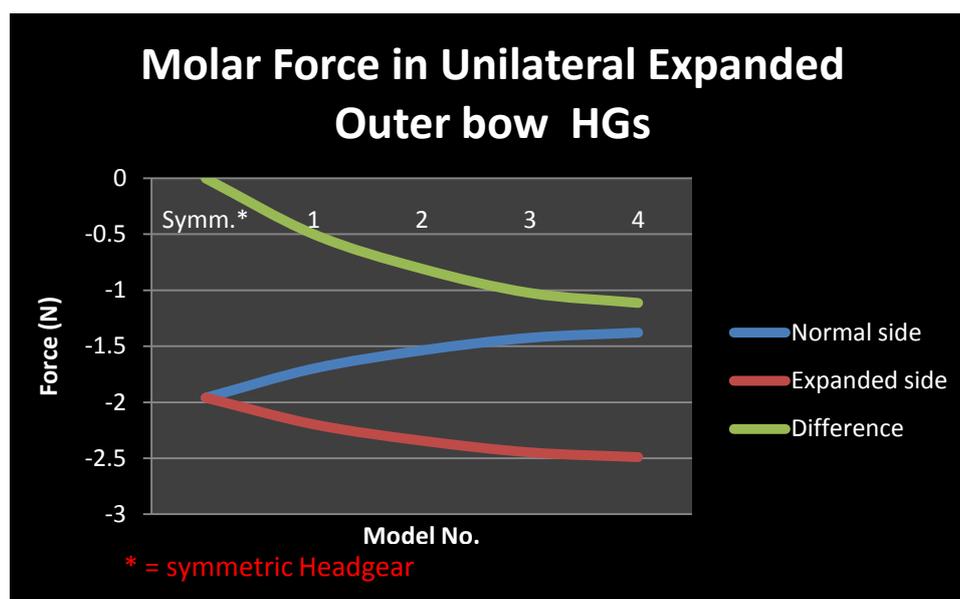


Fig 3. The produced molar forces in the normal side, the expanded side, and the difference of the forces.

Moment findings were the same as force findings in the symmetric model (-12.393 N.mm in the left side molar and 12.399 N.mm in the right side molar). A gradual decrease was shown in the expanded side molar moment between 11.171 N.mm and 9.906 N.mm in models 2 through 5.

An increase in the moment was shown from -13.434 N.mm in model 2 to -14.554 N.mm in the normal side molar (the negative sign shows the counterclockwise moment).

A  $\sum M \neq 0$  was found.

This residual moment had an ascending trend (Table 3) (Figure 4).

Table 1. The mechanical properties of the materials used in the models

	Young's Modulus (MPa)	Poisson's Ratio
<b>Tooth</b>	20300	0.26
<b>PDL</b>	0.667	0.49
<b>Spongy Bone</b>	13400	0.38
<b>Cortical Bone</b>	34000	0.26
<b>Stainless Steel</b>	200000	0.30

Table 2. Moment findings in the symmetric and asymmetric models (N.mm)

	Normal side	Expanded side	Difference
<b>Symm.*</b>	-1.9588	-1.9588	0
<b>1</b>	-1.6984	-2.1974	-0.499
<b>2</b>	-1.5371	-2.3444	-0.8073
<b>3</b>	-1.4248	-2.4486	-1.0238
<b>4</b>	-1.3789	-2.4916	-1.1127

Table 3. Moment findings in the symmetric and asymmetric models (N.mm)

	Normal side	Expanded side	Difference
<b>Symm.*</b>	-12.393	12.400	-0.007
<b>1</b>	-13.434	11.171	-2.263
<b>2</b>	-13.69	10.822	-2.868
<b>3</b>	-14.423	10.062	-4.361
<b>4</b>	-14.554	9.906	-4.648

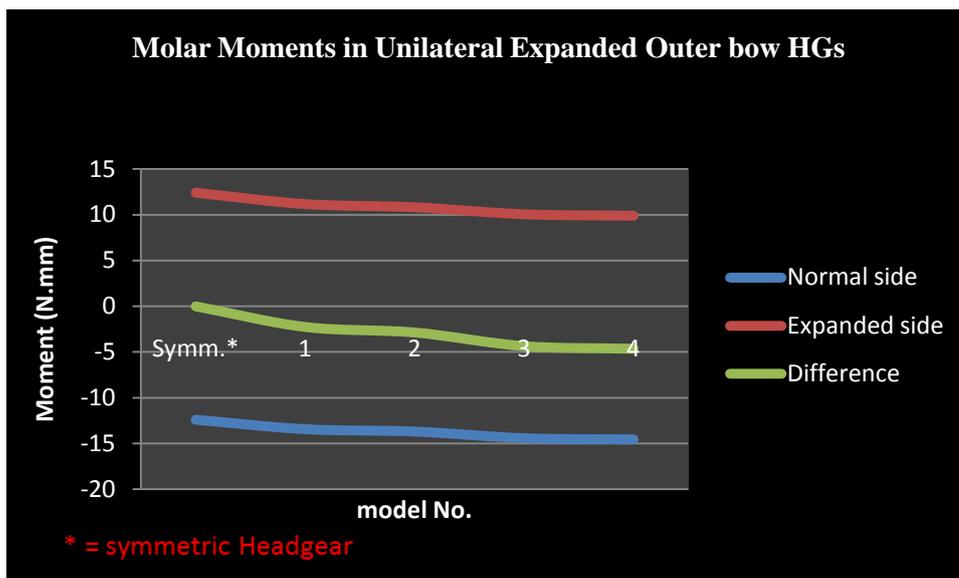


Fig 4. The produced moments in the normal side, the expanded side, and the difference of the moments.

## DISCUSSION

This study assessed a unilateral outer bow expanded headgear to produce an asymmetric distalizing force to molars. Producing asymmetric forces to the molars and also understanding the side effects are challenging for practitioners and researchers. Different methods have been studied and published to produce such asymmetric forces [13-17]. To analyze the force system of a headgear, tangent lines are drawn to the neck contour from the outer bow end points and continue posteriorly until crossing (Figure 2).

It must be necessarily drawn from different outer bow end positions. Different outer bow positions are obtained by: a) different outer bow lengths; b) expanding one outer bow end; and c) incorporating a swivel joint in an off-axis-inner/outer-bow-connection-point headgear. The decomposition of force is the same for an asymmetric headgear position and depends directly on the degree of deviation produced in the contact point of tangent lines, regardless of the manner of inducing such deviation. Evaluation of moments is the important part of this analysis.

When comparing different unilateral headgears, the only difference in the force system is the net moment.

Comparing different outer bow lengths and unilaterally expanded outer bow, the net moment in the system is an important part.

Finding the best position of the point of outer bow bend (to produce an effective asymmetric headgear) was another achievement of this study.

This was done analytically by drawing arcs with the center in the inner/outer bow connection point (the red point in Figure 2a) and also with the point of outer bow curvature (the green point in Figure 2a).

Comparing the curves, the green one was selected because of its ability to change the tangent line angle more than the other curve when viewed occlusally.

Viewing the curves drawn in Figure 2a (the green or the red one), it can be considered that outer bow end is moving away from its initial position, changing the tangent line angle up to a point and then the angle tends to return to its initial state (when viewed from the back of the neck in the mid-sagittal plane).

The maximum shift of the connection point between the tangent lines is the midpoint of the start and end of outer bow path (Figure 2a).

In this way, the increase of the force difference is not directly related to the increase of the expansion.

The force difference is increased up to the most prominent point of the path and will decrease afterwards. Considering the constant length of the outer bow, the position of the expanded outer bow end and the amount of deviation caused in the tangent line to the neck are mainly responsible for the produced unilateral force component. The path is in the form of a curve (actually, it is an arc with the center in a definite point on the outer bow). Thus, it can be visualized to move away from its neutral position up to a definite point and then moving back toward its initial position when viewed from the back of the neck.


If the expansion is not enough to resist the traction load, the tangent line to the neck will almost be the same as in the other side; thus producing more or less symmetric force decomposition and the moment will act to make the unilateral headgear. This situation can be summarized as "A small amount of unilateral expansion that can be neutralized by the neck strap can keep the intersection point of tangent lines along the mid-sagittal plane (receiving equal force component in both side molars) and providing a yawing moment for the system".

The asymmetric force production is not predictable in a unilateral outer bow expanded headgear. It is mainly based on the position of the outer bow after being flexed under the traction load and the difference produced in the angles of the neck tangent lines. This is a direct reflection of the flexibility provided by the outer bow. In this way, the role of the outer bow wire diameter is emphasized. Different molar distal forces are favorable to the clinician but the side effects are not ignorable and should be considered thoroughly.


Outer bow expanded headgears have a net yawing moment tending to rotate the dental arch clockwise or counter-clockwise when viewed occlusally. This force vector, when analyzed in combination with the moment difference present in the system, can interpret different pure molar distal movements in both sides of the arch. Moments tend to rotate the system around the vertical axis. The clockwise/counterclockwise direction of rotation is decided by the side of outer bow expansion. In an apico-occlusal view, the direction of rotation is clockwise when the right side outer bow arm is expanded and counter clockwise when the left side outer bow arm is expanded. Combining the effects of force system decomposition and the residual moment present, it will be almost impossible to determine the final position of the molars with geometric analytical methods. In the limited space present and considering the complexity of the displacement pattern, FEM is by far the most acceptable discipline of gathering data on the events. Several points have been mentioned regarding the headgear form and the importance of its outer-bow position and length [5-9]. The literature lacks any detailed published data on the outer bow expansion and its force system analysis considering the flexibility of outer and inner bows. Geramy and colleagues analyzed the mediolateral asymmetry in the molars being loaded by a symmetrical headgear [12].

They showed the difference in forces produced in molars, and explained some unwanted events in the process of treatment with a cervical headgear. These asymmetries can be considered to be unintentional.

Analyzing the asymmetries produced by the outer bow expansion and those produced by the difference in outer bow length, it is revealed that they have different natures. The laterally directed force vector is an unfavorable side effect, present in the headgears with different lengths of the outer bow [24] and is worsened by the presence of a net moment.

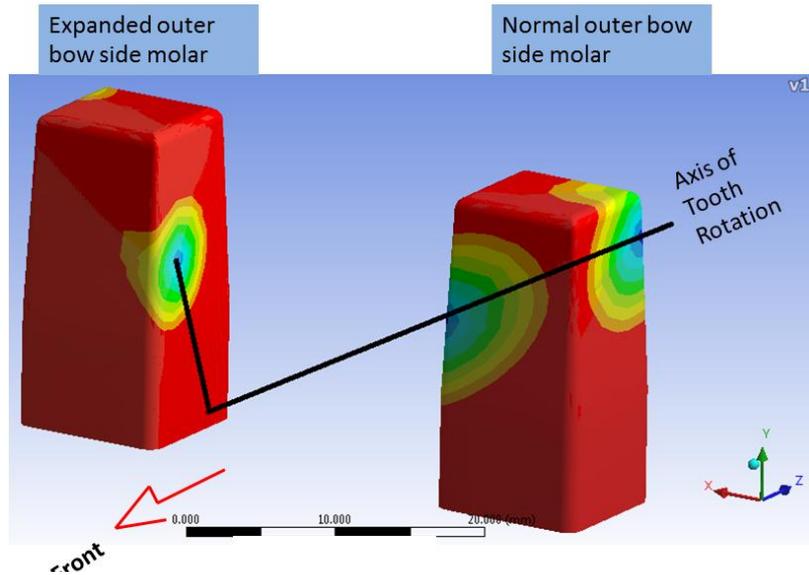

**Fig 5a.** Blocks to represent teeth to simplify presenting the manner of tooth movements when a unilateral expanded headgear is applied (the simplistic model can make it easier to find out how the teeth respond to the applied force system).

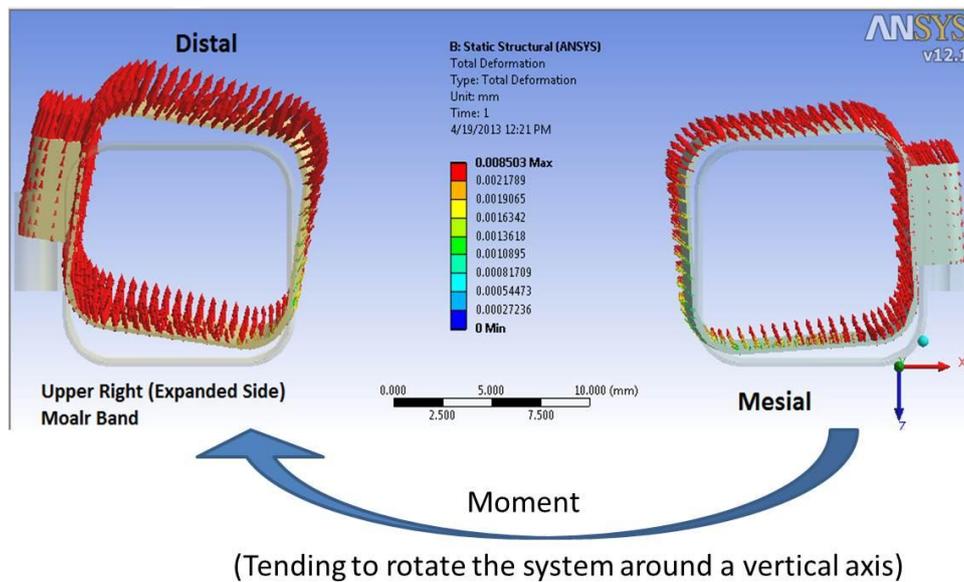

**Fig 5b.** The pattern of tooth movement shown in Figure 5a is viewed occlusally by tracing the band displacements. A distally driving force is shown to be combined with a yawing moment on molars.

As a whole, when reconsidering all findings, the response of upper molars can be summarized as a complex displacement shown in Figure 5a and b.

To simplify presenting the displacement in molars, an alternate model (model 6) was designed replacing molar teeth with cubic blocks

and the axis of movements was drawn based on the analysis of the numeric findings. The movements traced in molar bands are shown in Figure 5b.

Focusing on the pattern of molar band displacements, a distal movement of bands combined with a yaw can be noticed.

**CONCLUSION**

1. A residual yawing moment was found which tended to rotate upper arch (when applied to the entire arch) or upper molars (when applied to both side molars) clockwise/counter-clockwise according to the sign of the net moment (in an outer bow expansion head gear).
2. The amount of unilateral force produced by the outer bow expanded headgear increased up to a point and then decreased as explained.
3. In order to maximize the force difference in an outer bow expansion headgear, it is suggested to bend forward the outer bow with a center located in its curvature point (not the inner/outer bow connection point).
4. The net moment is expected to increase when the outer bow is expanded unilaterally and further increase as the expansion continues.

**REFERENCES**

- 1- Tweed CH. Clinical Orthodontics. St. Louis: Mosby Co.;1966.
- 2- Root L. The level anchorage system for correction of orthodontic malocclusion. Am J Orthod. 1981 Oct;80(4):395-410.
- 3- Marcotte MR. Biomechanics in orthodontics. Toronto: B.C. Decker Inc.; 1990.
- 4- Carriere J. Inverse anchorage technique in fixed orthodontics. Chicago: Quintessence books;1991.
- 5- Proffit WR, Fields HW, Sarver DM. Ackerman JL. Contemporary Orthodontics. 5<sup>th</sup> ed. Mosby Co,2013: 494.
- 6- Armstrong MM. Controlling the magnitude, direction, and duration of the extra oral force. Am J Orthod. 1971 Mar;59(3):217-43.
- 7- Oosthuizen L, Dijkman JFP, Evan WG. A mechanical appraisal of the Kloehn extra oral assembly. Angle Orthod. 1973 Jul;43(3):221-32.
- 8- Worms FW, Isaacson RJ, Speidle TM. Concept and classification of rotation and extra oral force systems. Angle Orthod. 1973 Oct;43(4):384-401.
- 9- Jacobson A. A key to the understanding of extra oral forces. Am J Orthod. 1979;75(4):361-86.
- 10- Hershey HG, Houghton CW, Burstone CJ. Unilateral face-bows: A theoretical and laboratory analysis. Am J Orthod. 1981;79(3):229-49.
- 11- Contasti GA, Legan HL. Biomechanical guidelines for the headgear application. J Clin Orthod. 1982 May;16(5):308-12.
- 12- Geramy A, Kizilova N, Terekhov L. Finite element method(FEM) analysis of the force systems produced by asymmetric inner head gear bows. Aust Orthod J. 2011 Nov;27(2):125-31.
- 13- Bratcher HJ, Muhi ZF, Randolph RG. Clinical measurement of distally directed headgear loading. Am J Orthod. 1985 Aug;88(2):125-32.
- 14- Yoshida N, Jost-Brinkmann PG, Miethke RR, Konig M, Yamada Y. An experimental evaluation of effects and side effects of asymmetric face-bows in the light of in-vivo measurements of initial tooth movements. Am J Orthod Dentofacial Orthop. 1998 May;113(5):558-66.
- 15- Chi L, Cheng M, Hershey HG, Nguyen T, Ko CC. Biomechanical reevaluation of orthodontic asymmetric headgear. Angle Orthod. 2012 Jul;82(4):682-90.
- 16- Squeff LR, Ruellas AC, Penedo ND, Elias CN, Sant'anna EF, Casaccia GR, et al. Asymmetric headgear for differential molar movement: a study using finite element analysis. J Orthod. 2009 Sep;36(3):145-51.
- 17- Brosh T, Portal S, Sarne O, Vardimon AD. Unequal outer and inner bow configurations: comparing 2 asymmetric headgear systems. Am J Orthod Dentofacial Orthop. 2005 Jul;128(1):68-75; discussion 75-7.
- 18- Geramy A. Moment/Force ratio and the center of rotation alteration:3D analysis by means of the FEM. J Dent, Shiraz University of Medical Sciences.2000;2(2):26-34.
- 19- Geramy A. Stress tensor modification in alveolar bone resorption: 3D analysis using

- finite element method. *Journal of Dentistry, Shiraz University of Medical Sciences* 2002; 3(3&4),39-49.
- 20- Geramy A, Adibrad M, Sahabi M. The effects of splinting periodontally compromised removable partial denture abutments on bone stress: a three-dimensional finite element study. *Journal of Dental Sciences* 2010; 5(1):1-7.
- 21- Geramy A, Ghadirian H. Comparison of methods used to correct a lingually tilted mandibular molar: 3-D analysis using the finite element method (FEM). *Aust Orthod J.* 2008 Nov;24(2):96-101.
- 22- Geramy A. The same amount of CRes displacement in various orthodontic tooth movements while the applied force is remained constant: 3D analysis using finite element method. *J Dent, Shiraz University of Medical Sciences* 2002; 3(1&2):59-65.
- 23- Geramy A. Cervical headgear force system: 3D analysis using finite element method. *J Dent, Shiraz University of Medical Sciences* 2000;2(3):21-30.
- 24- Nikolai RJ. *Bioengineering analysis of orthodontic mechanics.* Philadelphia: Lea &Febiger;1985.